## FEHLING TRADITION X PUNCHES

### 1) Components / Description




1. Punch body = shaft with fixed handle
2. Hex socket screw
3. Movable handle
4. Slider
5. Serial number
6. Hole
7. Guide surfaces/guide pins of the slider
8. Spring

### 2) Disassembly

1. Place the punch on a stable work surface for disassembly. Using the TXX-0X screwdriver (or the sterilisable TXW-9X screwdriver), turn the hex socket screw (2) clockwise and remove it from the threaded hole.

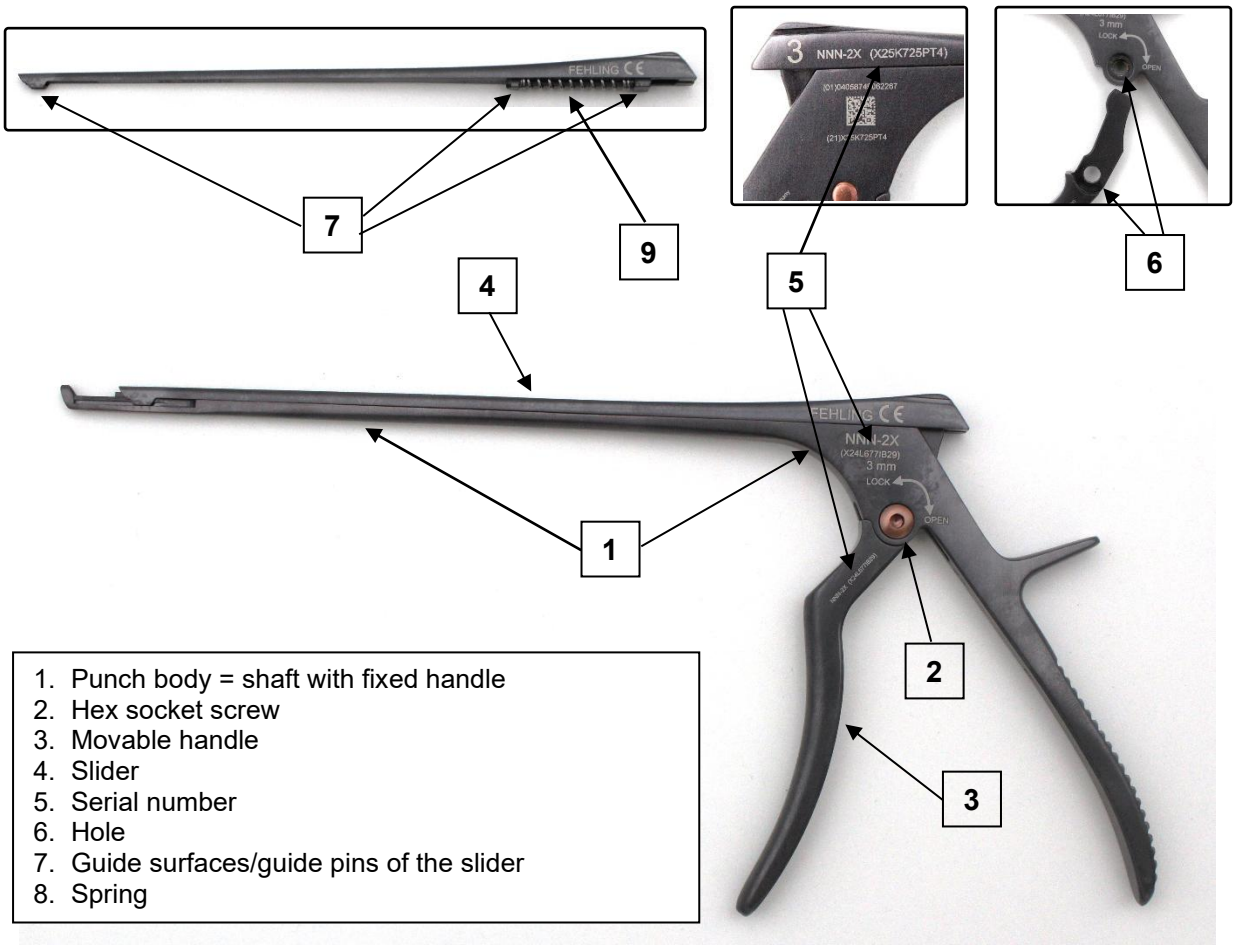

2. Pull the movable handle (3) downwards and separate it from the punch body (1). To facilitate unlocking, the slider (4) should be pushed simultaneously towards the footplate.



⚠ Removing the movable handle (3) automatically releases the slider (4).

3. The slider (4) can now be easily removed from the punch body (1).



4. Always reprocess the four individual parts together in the same container.



| | |
|---|---|
| ⚠ | For verification, the punch body (1), movable handle (3) and slider (4) are marked with the same serial number (5), for example X25K725PT4. Assemble only instrument parts with the same serial numbers (5). |

## 3) Assembly

1. Place the slider (4) with the spring (8) onto the shaft (1). At the same time, insert the guide surfaces/guide pins (7) of the slider (4) into the corresponding receptacles in the shaft (1).








| | |
|---|---|
| ⚠ | The guide surfaces/guide pins (7) of the slider (4) must fit into the corresponding receptacles in the shaft of the punch body (1). |

2. Slowly push the slider (4) towards the footplate until its end projects approximately 5 mm beyond the end of the shaft towards the footplate.



3. Keeping the slider (4) and shaft (1) in position, slide the movable handle (3) into the punch body (1). Ensure that the holes (6) in the movable handle (3) and punch body (1) line up precisely.



4. Using the TXX-0X screwdriver or the sterilisable TXW-9X screwdriver, turn the hex socket screw (2) anticlockwise into the designated threaded hole. Tighten the screw firmly without applying excessive force.



⚠ Do not overtighten!

5. After a functional test, the punch may be used again.



⚠

- This hex socket screw has a left-hand thread. Observe the direction of rotation when loosening and tightening the hex socket screws.
- Do not use excessive force when loosening and tightening the hex socket screw, as none is required. Excessive force when turning the screw may damage the hex socket profile.
- If damage to the hex socket profile or the screwdriver profile is detected, please replace the hex socket screw and screwdriver immediately or have them replaced by the manufacturer.
- The TXX-0X screwdriver can be washed with cold water and a mild detergent. It is not suitable for cleaning in hot water or steam sterilization at 134 °C.

| Symbols | | |
|---|---|---|
| Where shown on the medical device, medical device label or instructions for use, the symbols have the following meanings according to DIN EN ISO 15223-1: | | |
|  Manufacturer |  Consult instructions for use or consult electronic instructions for use |  Caution |
|  Catalogue number |  Batch code |  Serial number |
|  Medical device |  Unique device identifier |  0297 CE marking |
|  Oil can for points to be lubricated |  CE marking | |

| Manufacturer's contact information | | |
|---|---|---|
|  | FEHLING INSTRUMENTS GmbH<br>Seligenstädter Str. 100<br>63791 Karlstein, Germany<br>Tel.: +49 (0) 6188-9574-40<br>Fax: +49 (0) 6188-9574-45<br>E-mail: info@fehling-instruments.de<br>www.fehling-instruments.de |  |